

Optimising extraction and RT-qPCR-based detection of hepatitis E virus (HEV) from pork meat and products: Task Objectives

Task 1 Objective 1: Critical review

A critical review of studies on development of reverse transcriptase polymerase chain reaction (RT-PCR) based detection of HEV in foods was conducted in the initial stages of the project. The review described published HEV detection methods, with emphasis on those which have been successfully used in subsequent studies and surveys. The review focused on pork products and similar foodstuffs (e.g. from boar), but methods for detection of HEV in shellfish were summarised in an annex. One hundred and five papers were included in the review.

Various sample treatment procedures have been published, but it was difficult during the review to identify the most optimal method. Sample treatment procedures generally involved homogenisation, followed by nucleic acid extraction. The most commonly used procedures appear to be based on either tissue grinding or cell disruption.

Particularly in more recent studies, a sample process control (SPC) to monitor the efficiency of the extraction procedure has been included in the methods. In most cases, the SPC was a non-target virus added extraneously to the sample. Various SPC viruses have been used e.g., FCV, MNV, bacteriophage MS2. Some commercial analyses are performed using mengovirus (MgV). These viruses may not accurately reflect the characteristics of HEV and the effects of the extraction procedure on the virus.

RT-PCR assays have been used both qualitatively and quantitatively. It is clear from the review that the HEV RT-PCR of Jothikumar et al. (2006) is the best assay for use as the basis of a standardised method for analysis of pork products. It has been used as the basis for several subsequent methods for HEV detection in pork products, and is widely used in laboratories performing HEV diagnostics (Baylis et al., 2013). The assay has been reported as being more sensitive than alternative RT-PCRs (Mokhtari et al., 2013), and is capable of detecting at least 7 HEV genotypes including gts 1-4 (Giron-Callejas, 2015). An efficient RNA IAC exists for use in this assay (Diez-Valcarce et al., 2011b), which could also be used for calibration.

The complete critical review formed Deliverable 2 of the project. The review was subsequently published (Cook et al., 2022).

Task 2 Objective 2: Compilation of market share and consumption data of pork products in the UK.

The aim of this review was to help identify specific matrices for use in the HEVDETECT project, to reflect the most consumed pork products in the UK.

Three sets of data were acquired. The first set was from the NDNS (National Diet and Nutrition Survey) covering 2008 – 2016 (Bates et al 2014; Bates et al. 2016 and Roberts et al. 2018). From this information, it was concluded that the majority of the meats consumed, both carcass and processed, are cooked before consumption, while other products are not, e.g. chorizo, pepperami, etc. It was not possible to derive from the data how much of each of the listed

products are consumed.

The second dataset was derived from “Family Food datasets: countries and regions (CR) (updated with revised 2016/17 data and new 2017/18 data): Household purchases” (DEFRA, 2020), and shows the purchased quantities of household food & drink by Government Office Region and Country. These data show that uncooked pork sausages; cooked bacon and ham and uncooked bacon and ham rashers account for the majority of weekly purchases across all countries in the UK, followed by uncooked ham and bacon joints. The highest incidence of cases of HepE is in the South East and South West, which appears to coincide with the largest consumption of pork sausages. Indeed, it has previously been shown that the increased autochthonous incidence was first recognised in the S. West (Dalton et.al 2007). Further detailed statistical regression analysis is required to identify if any particular product is related in this data set.

The third dataset was obtained from Kantar UK – a data, insights and consulting company - and details the purchase of pork products by UK retailers during the year 2015 (kindly provided by Food Safety Scotland). This data set was not considered to be very useful, as there was no detailed breakdown of product type, and it related to purchased units of pork products by retailers, reiterating that the main types of products purchase fell into the chilled processed category.

In reviewing the data from the 3 datasets available, no conclusions could be arrived at with regard to specific product types consumed across the UK e.g., premium vs. economy pork sausages, salami, chorizo and hams. The general conclusion showed that pork sausages are one of the highest consumed products across the UK and consequently this matrix was included in the next phase of the project. The complete review of UK consumption data for pork products comprised Deliverable 3 of the project. The full report is in Appendix A.

Task 3 Objective 3: Development of an optimised HEV extraction procedure which delivers at least 1% efficiency of virus recovery, with a high level of consistency.

Following the information contained in the critical review (Deliverable 2), practical trials comparing the four selected viral RNA extraction protocols were carried out. The objective was to identify which method produced the greatest RNA yield recovery.

The matrices which were chosen were identified by the consumption data review (Deliverable 3).

3.1 Food selection and protocols

The first selected food matrices were sausages and pâté. Table 1 contains the information on the key ingredients that may affect the extraction efficiency. No minimum of porcine content was set as it is considerably variable.

Table 1: Key of food source and content of fat, carbohydrate, protein and porcine meat content as percentages.

Food source	Fat (per 100g)	Carbohydrate (per 100g)	Protein (per 100g)	Porcine Meat %
Low Grade Sausage (LGS)	14.3g	13.9g	13.5g	53%
High Grade Sausage (HGS)	21.9g	8.9g	16.6g	72%
Smooth Brussels Pâté (SBP)	22.5g	8.6g	9.6g	32%

Both GCU's and Campden BRI's own in-house protocols were tested as well as two described in the literature, Martin-Latil et, al, (2014) and Di Bartolo et al. (2015). These protocols are described in brief below:

3.2. Martin-Latil et al; (2014)

The protocol was followed as previously described by Martin-Latil et al, (2014) with the exclusion of the Mengovirus control. In brief, each 30mg sample was homogenised in 0.3ml of PBS using a stomacher apparatus and virus precipitated with 10% PEG 6000 and 0.3M NaCl. The sample was then centrifuged at 8000g for 30min at 4°C. The pellet was then resuspended in 100ul of PBS and vortexed with 1 mL of chloroform:butanol, 1:1 (v/v) to remove inhibitory substances from the virus extract. The suspension was then incubated for 5 min at room temperature, and centrifuged at 8000 g for 15 min at 4 °C. The upper aqueous phase containing the viruses was directly processed using the QiaAmp viral RNA kit according to the manufacturers protocol.

3.3. GCU in-house protocol

30mg (± 2 mg) was excised from sections of various pork meat products and spiked with 20,000 IU hepatitis E virus. Samples were then placed into tubes containing sterile glass beads and 600 μ l Buffer RLT from the Qiagen RNeasy kit. Each meat sample was homogenised at 50Hz for 2.5 minutes in the Qiagen TissueLyser LT. To remove debris, centrifugation (10,000 x G, 20 min 4°C). Succeeding tissue homogenisation, a Qiagen RNeasy kit was used to extract the total RNA content from all homogenates according to the manufacturer's instructions.

3.4. Di Bartolo et al. (2015)

250mg (± 2 mg) was excised from sections of various pork meat products and spiked with 20,000 IU hepatitis E virus. Samples were then placed into tubes containing sterile glass beads and 600 μ l Buffer RLT from the Qiagen RNeasy kit. Each meat sample was homogenised at a speed 4ms⁻¹ for 40s in the Qiagen TissueLyser LT and allowed to stand for 10 mins at room temperature. Following tissue homogenisation, a Qiagen RNeasy kit was used to extract the total RNA content from all homogenates according to the manufacturer's instructions.

3.5. Campden BRI in-house protocol

During this protocol, 2g was excised from sections of various pork meat products and spiked with 20,000 IU hepatitis E virus. Samples were then placed into IKA tubes containing 7ml of Trizol and subsequently homogenised for 6x 50s using an IKA Drive. Samples were then transferred to a 15m falcon tube and centrifuged at 10,000 g for 20 mins. 500ul of supernatant was then taken from the supernatant and taken forward for RNA extraction. RNA extraction was carried out using a Biomerieux Nuclisens Magnetic silica extraction kit according to manufacturers' instructions.

3.6. Detection of HEV by RT-qPCR

In addition to analysing various homogenisation and extraction techniques, 3 different Q-PCR protocols were tested to assess viral recovery. A primer set and cycling conditions were adopted from Jothikumar et. al (2006) and was used in conjunction with the Promega one step RT-PCR assay (Thermofisher Scientific) and the Qiagen viral Quantitect (Qiagen) for both one and two step formats respectively.

For the one step assay, in brief, 5ul of vRNA was added to the mastermix in a final volume of 25ul. Cycling conditions were; 45min at 45°C to allow for conversion into cDNA, then 95°C for 15 minutes followed by 45 PCR cycles of: 95°C for 10 seconds; 55°C for 20 seconds and 72°C for 15 seconds.

For two step RT-PCR assay, cDNA synthesis was undertaken with the use of Invitrogen Superscript III (Thermofisher Scientific) and was followed according to the manufacturer's protocols. In brief, 2ul of vRNA was mixed with 2pmol of gene specific primers, dNTPs and

nuclease free water. Samples were heated to 65°C for 5min then incubated on ice for at least 1min. To this, first-strand buffer, 0.1M DTT, RNase inhibitor and Superscript III RT were added as indicated by the instructions. The sample was incubated at 25°C for 5mins, then heated at 50°C for 45min. Reaction was inactivated by heating at 70°C for 15min. Amplification of the cDNA was carried out using the Quantitect PCR kit (Qiagen). Cycling conditions were identical to that of the Promega assay with the omission of the 45min incubation at 45°C.

The third assay additionally used to test all extracted viral RNA was a commercial CEERAM™ tools Hepatitis E Virus detection kit (Thermofisher Scientific). and was followed according to the manufacturer's protocol ([FT-KHEV-AN \(thermofisher.com\)](https://www.thermofisher.com/FT-KHEV-AN))([PU-KHEV-AN \(thermofisher.com\)](https://www.thermofisher.com/PU-KHEV-AN)). In brief, 5ul of viral RNA was added to the assay and cycling conditions were 10min at 45°C followed by 10min at 95°C then 40 cycles of 95°C for 15sec and 60°C for 45sec.

All RT-qPCR assays were quantified using HEV WHO international standards PEI and a synthetic RNA oligo (Integrated DNA Technologies). A DNA positive and negative control was also utilised in all RT-qPCR assays.


3.7. Results

3.7.1 Evaluation of three methods of PCR detection across all protocols selected.

Three types of pork foods were spiked with ~20,000 IU/ml of faecally derived hepatitis E virus (kindly provided by F Steinbach; APHA). Low grade sausage (LGS - low % pork meat), High grade sausage (HGS – high % pork meat) and Smooth Brussels Pâté (SBP) were spiked with HEV prior to homogenisation and extraction. The four methods, as described in section 3.2 – 3.5, were carried out and the isolated HEV viral RNA was then quantified using the three different RT-qPCR assays. Additionally, sample process controls were utilised and introduced before homogenisation (PBSV1 &2) and after homogenisation (PBSV3). No virus controls were also utilised to ensure there was no infected tissue prior to spiking.

Comparison of assay Ct values found that all four protocols showed consistent recoveries across all types of samples tested but were not always detected by all of the RT-qPCR assays (Figure 1 A-D). The commercial Ceeram™ HEV detection kit gave slightly lower Ct values than that of the 1 and 2-step RT-qPCRs, but consistently demonstrated a positive value for each assay as did the 2-step RT-qPCR, with the exception of PBSV3 (Figure 1A). The 1-step assay frequently showed a lack of detection in three of the four protocols. Only CBRI protocol gave consistent detection using all PCR methods (Figure 1D). This suggested that the 1-step assay may not be as consistent as the other two and that the commercial Ceeram assay was most likely to detect viral RNA.


Figure 1: Detection of HEV post extraction by RT-qPCR HEV. Values are represented as cyclic Thresholds (Ct). Ct of HEV RNA isolated (A) using Martin-Latil et al. (2014) protocol, (B) using GCU protocol. (C) using Di Bartolo et al. (2015) protocol and (D) using Campden BRI protocol. RNA extracted from each protocol was tested using 3 different RT-qPCR assays: 1-step (Blue); Ceeram (Orange) and 2-step (Grey).



3.72 Evaluation of percentage recovery of HEV in the protocols selected.

Recovery of viral RNA was presented as a percentage of the input virus to establish that the >1% recovery detection was met by the protocols used, including the detection method. Prior to this, the average percentage recovery for PBSV1 and PBSV2 was evaluated. PBSV1 was the control for the homogenisation and extraction protocol where we wanted to establish the recovery of both HEV and the SPCV post treatment. PBSV2 was the control where the samples were not subjected to any homogenisation or extraction and were a direct recovery of the virus input which essentially should be circa 100%. Figure 2 summarises the data for the PBSV controls for each protocol and each PCR method.

Figure 2: PBSV average percentage recovery for HEV and SPCV for all protocols and detection methods.

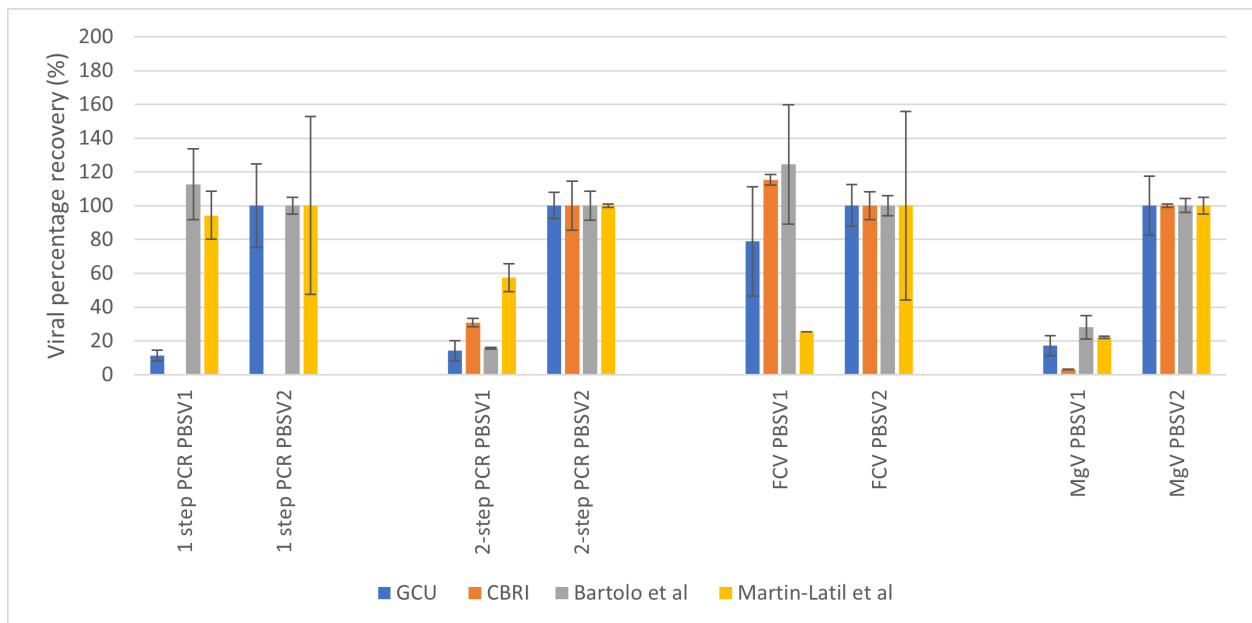

In summary, it was found that again, the 2 step PCR method was the most effective and consistent at detection of HEV. Martin-Latil, et al (2015) gave the best recovery post extraction with the other three methods equivalent. The 2 step PCR method also gave the most accurate return on the 100% PBSV2 values for all protocols and a >1% recovery for all protocols after extraction. For the SPCVs, FCV recovery was poor for the method by Martin Latil, et al (2015) and MgV recovery was the poorest for the in-house CBRI protocol. In terms of utilising FCV or MgV as SPCV controls, the methods by GCU and Di Bartolo et al, (2014) were deemed the best in order to permit a choice for others using the assay.

Table 2 summarises the data and recovery values for each of the four protocols. All protocols exceeded the >1% threshold required. However, there were inconsistencies noted in the combinations of extraction and detection. For example, the GCU protocol worked best with the commercial assay, as did all of the assays with the Martin-Latil et al, (2014) protocol giving the highest percentage recovery of virus compared to input material albeit there were several anomalies in the data sets. The 1-step RT-qPCR frequently gave no value suggesting that it is not very reproducible. The 2-step RT-qPCR also worked well in all protocols with a few exceptions. Overall, the commercial assay was deemed the best detection protocol on this basis, however, costs are prohibitive if this is to be an assay that is accessible to all.

In conclusion, the one step PCR was not suitable for consistent detection based on the data. The CeeramTM assay was the most consistent but the cost for general use is prohibitive and the aim was to identify a simple cost-effective detection method.

All methods performed well with the 2 step PCR protocol. One aim was that the final protocol should not include any hazardous reagents and should have the simplest method to allow it to be utilised by any end user. Based on this, the GCU, Di Bartolo, et al (2015), and Martin-Latil, et al (2014) were considered the safest extraction procedures. However, the latter protocol did not show good recovery for the SPCV. A full assessment of HEV recovery was carried out on all four protocols for comparison (Appendix B), however, the data for the in-house GCU protocol and that by Di Bartolo et al, (2015) are reported here for comparison (Table 2).

Table 2: HEV recovery from pork sausage (high and low grade) and smooth pâté using four extraction and three different detection methods. All assays were repeated twice as two biological replicates then technical replicates in the PCR (n=2).

Protocol	Source	Extraction buffer	1 step RT-qPCR Mean CT ad SD	2-step RT-qPCR Mean CT and SD	Ceeram Mean CT and SD	1 step RT-qPCR % recovery	2 step RT-qPCR % recovery	Ceeram % recovery
GCU	Low grade Pork sausage 1	RLT lysis	35.184/0.338	38.438/0.118	34.871/0.382	64.16	27.72	5.49
GCU	Low grade Pork sausage 2	RLT lysis	35.154/0.224	39.402/0.000	35.243/0.485	65.05	12.67	4.23
GCU	High grade Pork sausage 1	RLT lysis	34.333/0.510	37.995/0.772	34.461/1.264	124.5	43.54	8.85
GCU	High grade Pork sausage 2	RLT lysis	32.715/0.049	35.691/0.005	31.968/0.041	407.5	256.33	44.74
GCU	Smooth Brussels Pâté 1	RLT lysis	0/0	36.867/0.484	33.738/0.651	0.000	102.63	13
GCU	Smooth Brussels Pâté 2	RLT lysis	0/0	35.622/0.025	32.777/0.039	0.000	271.1	24.79
Di Bartolo et al (2015)	Low grade Pork sausage 1	RLT lysis	38.547/0	34.423/0.096	34.948/0.118	9.82	122.39	8.94
Di Bartolo et al (2015)	Low grade Pork sausage 2	RLT lysis	33.452/0.067	35.521/0.199	31.945/0.012	355.75	59.62	64.59
Di Bartolo et al (2015)	High grade Pork sausage 1	RLT lysis	36.713/0.220	32.260/0.005	31.135/0.042	35.97	508.27	110.37
Di Bartolo et al (2015)	High grade Pork sausage 2	RLT lysis	37.411/0.199	34.933/0.000	33.669/0.246	21.97	87.41	20.82
Di Bartolo et al (2015)	Smooth Brussels Pâté 1	RLT lysis	0.000/0.000	32.849/0.097	32.709/0.174	0.000	345.11	39.13
Di Bartolo et al (2015)	Smooth Brussels Pâté 2	RLT lysis	0.000/0.000	34.709/0.044	32.033/0.074	0.000	101.3	60.98

3.73 Evaluation of recovery in additional pork products.

Five types of pork meat were spiked with ~20,000 IU/ml of faecally derived HEV, 3.25x10⁶ pfu/ml FCV/MS2 and 2.76x10⁵ pfu/ul of Mengovirus. The following meats were Low grade sausage (LGS), High grade sausage (HGS) and Smooth Brussels pâté (SBP), Porcine Liver (LIV) and Salami (SAL). Succeeding the spiking of the different meat samples, the two different homogenisation/RNA extractions techniques were undertaken (Figures 3 and 4). The isolated HEV viral RNA was then quantified, again, using the two different RT-qPCR assays.

Figure 3: Percentage recovery of HEV in 5 different pork derived products using the in-house GCU protocol. LGS = low grade sausage, HGS = high grade sausage, SBP = smooth brussels pate, LIV – liver, SAL = salami; PBSV1= samples spiked with SPCV and HEV then homogenised and extracted and PBSV2 = no homogenisation or extraction treatment. FCV and MgV (Mengo) represent the two SPCV controls spiked in with the samples. Error bars indicate the SD (n=4).





Figure 4: Percentage recovery of HEV in 5 different pork derived products using the protocol by Di Bartolo et al (2015). LGS = low grade sausage, HGS = high grade sausage, SBP = smooth brussels pate, LIV – liver, SAL = salami; PBSV1= samples spiked with SPCV and HEV then homogenised and extracted and PBSV2 = no homogenisation or extraction treatment. FCV and MgV represent the two SPCV controls spiked in with the samples. Error bars indicate the SD (n=4).



For the further analysis using pork liver and salami, in-house GCU protocol showed recovery for HEV above the threshold of 1% in all foods tested for both PCR methods. In comparison, the method by Di Bartolo et al (2015) gave no recovery in the salami homogenate for either PCR method and in the liver homogenate, only the one step PCR method gave a recovery.

In terms of recovery of virus, we see variable results across the literature with the reporting not always consistent. This made it difficult to determine the best assay without a direct comparison in a number of pork derived food products.

More recent reports show that the use of ultracentrifugation and filtration can aid recovery (Harrison et al, 2021), however, some of these approaches are not accessible to all. In terms of recovery, the in-house GCU protocol gave an average of 15% for LGS, 22% for HGS, 47% for SBP, 48% for liver and around 5% for salami. Due to the variability in reporting in the literature it is not always possible to compare recoveries, however, compared to previously reported

recoveries, these are considered high (Table 3).

Table 3. Example published methods for detection of HEV in pork products presented as percentage recovery. PBS = phosphate buffered saline; RLT =RNeasy lysis buffer (supplied by Qiagen).

Reference	Meat Source	Extraction Buffer	Virus Concentration Step	HEV Recovery %	SPCV Recovery %
Colson et al, 2010	Wild boar	PBS	No	0.6	ND
DiBartolo et al, 2012	Pork sausage	RLT Lysis	No	0.04	ND
DiBartolo et al, 2015	Pork sausage	RLT Lysis	No	ND	18
Martin-Latil et al, 2015	Figateli/sausage	Distilled Water	Yes	13.1/2.9	18.4/3.9
Szabo et al, 2015	Pork sausage	Trizol	Yes	4.9	11.2


Consumption of pork products that may contain raw elements and the ability to detect HEV in these food matrices is of high importance. Indeed, due to the complex nature of these matrices it is anticipated that a higher recovery would be seen in more homogeneous matrices. Szabo et al, (2015) demonstrated recovery from raw salami sausage however the method utilised chloroform and Tri reagent in the protocol (Szabo et al, 2015). Our aim here was to ensure the design of a protocol with a full suite of controls without any hazardous reagents.

Overall, this confirmed that the protocol being taken forward to Task 5 would be the GCU protocol as it was the most consistent and demonstrated detection of HEV in all food homogenates tested.

Task 4 Objective 4: Development of an optimized, quantitative RT-PCR assay for detection of HEV, incorporating a full suite of controls

To ensure that all assays and methods developed were fully controlled we have specified those that must be included in any extraction and detection assay. It was clear from Task 3 that the use of a 2 step PCR assay would be the most cost effective and consistent. The addition of SPCV also controlled for loss of material during the extraction process. In addition to the negative controls, an important analytical control in molecular amplification-based methods is an internal amplification control (IAC), which should be included in each reaction mixture. An IAC is a nontarget nucleic acid sequence which is coamplified simultaneously with the target sequence. This is necessary to provide an internal PCR control for inhibition. The IAC was designed based on Diez-Valcarce et al (2011). The IAC was then tested for amplification and a dilution curve created to determine the LOD (Figure 5). For future PCRs, the IAC was used to give a Ct 33-36.

Figure 5:



The IAC was also assessed to ensure that it functioned in the presence of food extracts and there was no detrimental effect on virus detection.

All samples were run with and without an IAC post extraction on the PCR (Table 4A and B). The selected method was tested with the IAC along with another method to confirm that the IAC was indeed suitable for use. (Figure 6). The IAC gave consistent results in both methods assessed and confirmed that it was suitable for use in task 5.

Table 4A: Ct values for HEV detection in liver sample with and without the IAC present. NTC = no template control. Liver 1 and 2 are biological replicates. The mean Ct is calculated from technical replicates for each one(n=2).


Sample ID	Mean Ct HEV 1	Mean Ct HEV 2	Mean Ct IAC 1	Mean CT IAC 2	Mean Ct MgV 1	Mean Ct MgV 2
Liver 1	35.92	35.54	36.11	33.96	34.23	32.57
Liver 2	UD	33.58	34.47	33.88	33.31	32.31
NTC	UD	UD	34.04	UD	UD	UD

Table 4B: Confirmation of MgV SPCV standard curve values. R2 =0.96. All NTC were UD.

MgV dilution	Mean Ct
10%	23.35
1%	25.82
0.1%	29.07
0.01%	32.55

Overall, the IAC was found to have no impact on the HEV detection or that of the SPCV. One of the liver samples gave no signal in the PCR (Liver 1 PCR replicate 1). These samples had been previously freeze-thawed so it was suspected that it may be due to loss of virus in this process that gave a negative result in the assay. This IAC showed that the homogenisation and extraction method did not result in the presence of any inhibitors from all 5 food sources and was taken forward for use in Task 5.

Figure 6: Effect of IAC on amplification of the target using two methods; the in-house GCU and CBRI protocols.



Task 5 Objective 5: Inter-laboratory evaluation of the method.

To verify that the final method was repeatable and reproducible, a collaborative trial was performed with partners from the UK and Europe. In the trial, the samples were pig liver spiked with HEV genotype 3. The trial was conducted “blind” by each participant. Seven laboratories participated in the trial. They comprised Fera Science Limited (Fera, UK), Campden BRI (CBRI, UK), Animal and Plant Health Agency (APHA, UK), Glasgow Caledonian University (GCU, UK), Istituto Superiore di Sanita (ISS, Italy), University of Burgos (UoB, Spain) and The French Agency for Food, Environmental and Occupational Health and Safety (ANSES, France). Each participant was provided with a personalised standard operating procedure (SOP) for performance of this trial.

Trial materials comprised pork liver artificially contaminated with HEV at three levels - . 6×10^4 genome copies (gc) HEV (HIGH level), 6×10^3 gc HEV (MEDIUM level), and 6×10^2 gc HEV (LOW level). Uncontaminated (BLANK) liver samples were also included. All samples contained 6.71×10^6 gc MgV as SPCV.

Each participant was sent extraction and RTPCR reagents necessary to perform the method. The trial materials were couriered on dry ice to the participants.

Raw data were reported by each participant to the trial coordinators, who translated the codes and analysed the data. The trial coordinators checked each participants data including the log and linear amplification plots for the HEV assay (including the IACs), the log and linear amplification plots for the MgV assay and the instrument data (where possible). The checks were performed to ensure only reaction signals indicative of correct amplification were included in the subsequent evaluation. No Ct cut-off criterion was applied. Interpretation of the results followed the principles outlined by D’Agostino et al. (2011). When a participant reported at least one of the

replicates for the HEV assay (Neat and 1:10) was positive, the sample was recorded as HEV-positive. When a participant reported that all replicate HEV assays (Neat and 1:10) were negative, but the IAC and the MgV were detected, the sample was recorded as HEV-negative. If the MgV or the IAC were not detected in a HEV negative sample, the analysis was recorded as having failed. If a positive HEV signal was found in the PCR-ve control, then that participant's results were excluded from the trial.

The data were statistically analysed according to the recommendations of Scotter et al. (2001) and by the methods of Langton et al. (2002).

Table 5 shows the diagnostic specificity, diagnostic sensitivity, positive and negative predictive values, accordance and concordance values and the concordance odds ratio for the collaborative trial of the analytical method for the detection of HEV in pork liver.

The repeatability and reproducibility of the HEV DETECT method were evaluated by determining the accordance, concordance, and concordance odds ratio (COR) of the trial data. In plain language, accordance is the probability of getting an identical result from two unknown samples analysed in the same laboratory, in other words the repeatability. Concordance is the probability of getting the same result from two identical samples, where one is analysed in one laboratory and the other is analysed in a different laboratory: in other words, reproducibility. The COR merges repeatability and reproducibility: a COR of ≥ 1.00 indicates that two samples sent to different laboratories will probably produce the same result that would be obtained if the same two samples were analyzed by a single laboratory. A COR significantly > 1.00 indicates that variability between laboratories is greater than the variation within a single laboratory. In this collaborative trial, the CORs for the HEV-contaminated and the uncontaminated samples were within the 95% confidence intervals and therefore not significantly > 1.00 . Thus, the HEV DETECT method was just as reproducible between laboratories as it was repeatable within a laboratory.

The HEV DETECT method contains an IAC. One participant laboratory reported one failed analysis where the IAC signal did not appear. All other IAC signals were present. In the HEV DETECT method, the IAC was not used to determine levels of inhibition, as in the method to detect norovirus and hepatitis A virus described in ISO15216 (Anon. 2019). Rather, the presence of an IAC signal demonstrated that the amplification of the RT-PCR performed correctly.

The HEV DETECT method produced mean recoveries of 4.5% - 130%. One sample produced a recovery of 311%; in a similar study (Trojnar et al., 2020) one sample produced a recovery of 303.1%. Trojnar et al. (2020) observed higher recoveries in their diluted samples than in their neat samples, and this was also observed in the HEV DETECT trial. It is currently difficult to explain the reasons for recoveries above 100%.

Table 5: Statistical evaluation of the data obtained from the collaborative trial

Cont. level	Sensitivity (%)	Specificity (%)	Positive Predictive Value	Negative Predictive Value	Accordance (%)	Concordance (%)	Concordance odds ratio (COR)
All HEV spiked samples*	83.3 (68.1, 92.1)	-	93.8 (79.9, 98.3)	-	82.2 (64.4, 100.0)	69.6 (48.9, 100.0)	2.02 (1.0, 2.92)
BLANK	-	83.3 (55.2, 95.3)	-	62.5 (38.6, 81.5)	66.7 (33.3, 100.0)	70.0 (53.3, 100.0)	0.86 (0.44, 1.0)

*LOW, MEDIUM and HIGH results combined. Values in parentheses are the lower and upper 95% confidence intervals

It was noted that several of the trial kits which were sent by courier to the participating laboratories failed to be delivered in their original frozen condition. For the kits sent to European laboratories, the current status of the UK as a third country resulted in delays at EU Customs /

Border control causing in some cases several weeks delay. However, this did not appear to have a detrimental effect on the trial.

There is currently debate within the scientific community regarding the interpretation of “high” Ct values e.g., above 40. In the Jothikumar et al (2006) assay upon which the method is based, a cut-off value of Ct45 was used. All samples in the HEV DETECT trial produced Ct values <45. In the collaborative trial reported by Trojnar et al (2020) it was reported that some samples including “high” contamination levels produced Ct values >40; values below Ct50 were considered acceptable. In the HEV DETECT trial several samples displayed Ct values above 40. All these values were individually checked and were judged to represent amplification of target sequences.

In conclusion, the collaborative trial was performed successfully and the resulting data demonstrates the utility, repeatability and reproducibility of the HEV DETECT method. The full report of the trial comprised Deliverable 12.